

## Supporting Information

### Scanning electrochemical flow cell with online mass spectroscopy for accelerated screening of carbon dioxide reduction electrocatalysts

Yungchieh Lai, Ryan J.R. Jones, Yu Wang, Lan Zhou, and John M. Gregoire

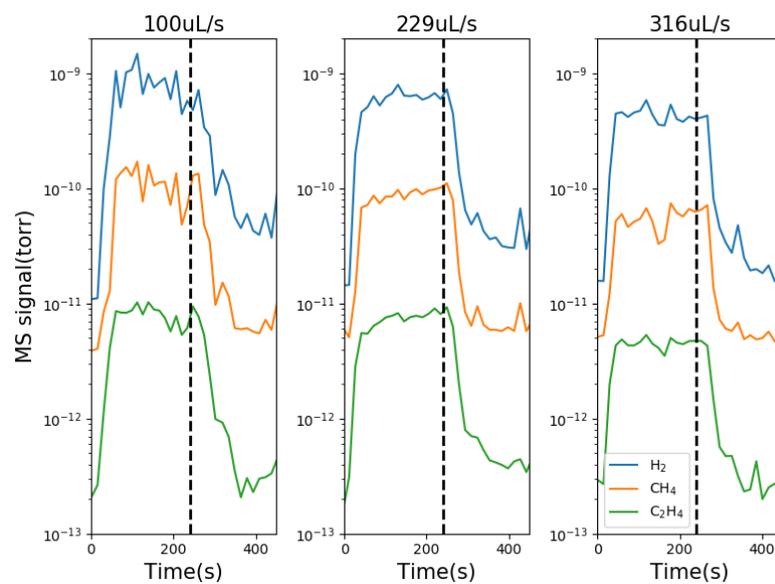


Figure S1. Effect of electrolyte flow rate. Chronoamperometry (CA) was carried out over a copper foil for 240 (s) at different flow rates. The black dashed line indicates where the CA ends.